

## Central Lancashire Online Knowledge (CLOK)

Title	Quantifying varus thrust in knee osteoarthritis using wearable inertial sensors: A proof of concept
Type	Article
URL	<a href="https://clock.uclan.ac.uk/35822/">https://clock.uclan.ac.uk/35822/</a>
DOI	<a href="https://doi.org/10.1016/j.clinbiomech.2020.105232">https://doi.org/10.1016/j.clinbiomech.2020.105232</a>
Date	2020
Citation	Costello, Kerry E, Eigenbrot, Samantha, Geronimo, Alex, Guermazi, Ali, Felson, David T, Richards, James and Kumar, Deepak (2020) Quantifying varus thrust in knee osteoarthritis using wearable inertial sensors: A proof of concept. <i>Clinical Biomechanics</i> , 80. p. 105232. ISSN 0268-0033
Creators	Costello, Kerry E, Eigenbrot, Samantha, Geronimo, Alex, Guermazi, Ali, Felson, David T, Richards, James and Kumar, Deepak

It is advisable to refer to the publisher's version if you intend to cite from the work.  
<https://doi.org/10.1016/j.clinbiomech.2020.105232>

For information about Research at UCLan please go to <http://www.uclan.ac.uk/research/>

All outputs in CLOK are protected by Intellectual Property Rights law, including Copyright law. Copyright, IPR and Moral Rights for the works on this site are retained by the individual authors and/or other copyright owners. Terms and conditions for use of this material are defined in the <http://clock.uclan.ac.uk/policies/>

1 Title: Quantifying varus thrust in knee osteoarthritis using wearable inertial sensors: a proof of concept

2  
3 Authors: \*Kerry E. Costello, PhD<sup>a,b</sup>, \*Samantha Eigenbrot, MS<sup>a</sup>, Alex Geronimo, MS<sup>a</sup>, Ali Guermazi, MD,  
4 PhD<sup>b,c</sup>, David T. Felson, MD, MPH<sup>a,b</sup>, Jim Richards, PhD<sup>d</sup>, Deepak Kumar, PT, PhD<sup>a,b</sup>

5  
6 Affiliations:

7 <sup>a</sup> Department of Physical Therapy & Athletic Training, Boston University College of Health &  
8 Rehabilitation Sciences: Sargent College, Boston, MA, USA

9 <sup>b</sup> Division of Rheumatology, Department of Medicine, Boston University School of Medicine, Boston, MA,  
10 USA

11 <sup>c</sup> Department of Radiology, VA Boston Healthcare System, Boston University School of Medicine, Boston,  
12 MA, USA

13 <sup>d</sup> Allied Health Research Unit, School of Sport and Health Sciences, University of Central Lancashire,  
14 Preston, UK

15  
16 Corresponding author: Deepak Kumar, 635 Commonwealth Ave, Boston MA, 02215, USA,  
17 kumard@bu.edu

18  
19 Declarations of interest: Ali Guermazi is Shareholder of BICL, LLC and Consultant to AstraZeneca,  
20 MerckSerono, TissueGene, Pfizer, Roche and Galapagos. Other authors declare no conflict of interest.

21  
22 Word count (abstract): 249; Word count (main text): 3852

## Abstract

*Background:* Varus thrust during walking, visualized as excessive frontal plane knee motion during weight acceptance, is a modifiable risk factor for progression of knee osteoarthritis. However, visual assessment does not capture thrust severity and quantification with optical motion capture is often not feasible. Inertial sensors may provide a convenient alternative to optical motion capture. This proof-of-concept study sought to compare wearable inertial sensors to optical motion capture for the quantification of varus thrust.

*Methods:* Twenty-six participants with medial knee osteoarthritis underwent gait analysis at self-selected and fast speeds. Linear regression with generalized estimating equations assessed associations between peak knee adduction velocity or knee adduction excursion from optical motion capture and peak thigh or shank adduction velocity from two inertial sensors on the lower limb. Relationships between inertial measures and peak external knee adduction moment were assessed as a secondary aim.

*Findings:* Both thigh and shank inertial sensor measures were associated with the optical motion capture measures for both speeds ( $P < 0.001$  to  $P = 0.020$ ), with the thigh measures having less variability than the shank. After accounting for age, sex, body mass index, radiographic severity, and limb alignment, thigh adduction velocity was also associated with knee adduction moment at both speeds (both  $P < 0.001$ ).

*Interpretation:* An inertial sensor placed on the mid-thigh can quantify varus thrust in people with medial knee osteoarthritis without the need for optical motion capture. This single sensor may be useful for risk screening or evaluating the effects of interventions in large samples.

**Keywords:** angular velocity, gyroscope, motion capture, adduction

## 1. Introduction

Knee osteoarthritis (OA) is a leading cause of disability among older adults<sup>1</sup> and most commonly affects the medial tibiofemoral compartment of the knee joint<sup>2</sup>. While age, sex, genetics, and other non-modifiable factors have been implicated in OA pathogenesis, gait patterns leading to increased or abnormal biomechanical joint loading also play a role and are frequently targeted in interventions<sup>3</sup>. A common gait abnormality in people with medial knee OA is varus thrust, an excessive 'bowing-out' knee motion in the frontal-plane during ambulation as the limb accepts weight with a return towards a more neutral alignment in late stance and swing<sup>4,5</sup>. Varus thrust has been reported to be present in 12% to 46% of individuals with medial knee OA and has been associated with radiographic disease severity<sup>6</sup> and progression<sup>5</sup>. Cross-sectionally, those with varus thrust have a five-times greater odds for higher pain during walking and standing than those without it<sup>7</sup>. Individuals with knee OA who exhibit varus thrust also exhibit greater peak external knee adduction moments (EKAM) during gait<sup>5</sup>, an indication of medial tibiofemoral load<sup>8</sup> which has been reported to be a risk factor for future OA progression<sup>9</sup>. Thus, interventions to reduce varus thrust may lead to reduced pain and slow structural worsening in individuals with medial compartment knee OA.

To aid in the development of effective interventions, it is important to accurately and reliably identify the presence of varus thrust. Typically, varus thrust is assessed through a subjective, visual evaluation of walking<sup>5-7,10-14</sup>. While these assessments are used clinically, they only provide a dichotomous categorization (present/absent) without any indication of severity. To overcome this limitation, optical motion capture has been used to objectively quantify biomechanical parameters as surrogate measures of varus thrust<sup>5,6,15-21</sup>, including knee adduction velocity<sup>6</sup> and knee adduction angular excursion<sup>21</sup>. However, while optical motion capture provides detailed information on joint kinematics and kinetics, these systems require expensive equipment, time-consuming data collections run by skilled technicians, and a large calibrated measurement volume, making their clinical use

infeasible. Additionally, analyses conducted in a laboratory environment do not always reflect typical walking in real-world settings<sup>22</sup>. In contrast, small, low-cost wearable inertial sensors have become increasingly popular for collecting biomechanical data in free-living conditions and may provide a convenient alternative to optical motion capture systems for quantifying varus thrust<sup>23</sup>.

The primary aim of this study was to compare data from a single wearable inertial sensor to surrogate measures of varus thrust captured using optical motion capture technology during self-selected and fast speed walking in individuals with medial compartment knee osteoarthritis. We hypothesized that measures of frontal plane segment velocity from single inertial sensors placed on the thigh or shank would be significantly associated with measures from optical motion capture based on previously reported agreement between inertial sensor and optical motion capture kinematic and kinetic measures<sup>24,25</sup>. For a secondary aim, we hypothesized that the inertial sensor measures would be associated with EKAM after adjusting for confounders.

## **2. Methods**

### *2.1. Participants*

Participants were recruited using advertisements online and in local newspapers from October 2017 to May 2019. Inclusion criteria were age between 45-80 years, body mass index (BMI)  $\leq 40 \text{ kg/m}^2$ , and at least one knee meeting the American College of Rheumatology clinical or radiographic criteria for knee OA<sup>26</sup> with primarily medial tibiofemoral compartment involvement (medial joint space narrowing identified from weight bearing knee radiographs). Exclusion criteria were regular use of a walking aid, inflammatory arthritis, lower limb total joint replacement, neurological conditions, muscular disease, or other conditions/treatments affecting gait. This study was approved by the Boston University Institutional Review Board, Boston, USA, and all individuals provided written informed consent prior to radiographic screening and data collection.

## *2.2. Radiographs and Assessment of Symptoms*

All participants underwent three radiographs: (1) bilateral weight-bearing posterior-anterior flexed knee radiograph using a Synaflexer positioning frame (BioClinica, Princeton, NJ, USA) for assessment of Kellgren-Lawrence grade (KLG) and assessment of medial and lateral tibiofemoral compartment involvement based on the Osteoarthritis Research Society International (OARSI) atlas, (2) bilateral knee sunrise view for assessment of patellofemoral involvement, and (3) bilateral standing long limb view for measurement of static mechanical axis alignment. An experienced clinician assessed OA severity (KLG) and determined the most involved compartment (medial or lateral) for each knee. Inter-reader reliability for KLG of 0.79 has been reported previously<sup>27</sup>. Static alignment was calculated using OsiriX open-source software ([www.osirixviewer.com](http://www.osirixviewer.com))<sup>28</sup> as the angle formed by the intersection of the line between the center of the femoral head and midpoint of the femoral epicondyles, and the line between the midpoint of the femoral epicondyles and midpoint of the malleoli. All participants also completed the Knee Injury and Osteoarthritis Outcome Score (KOOS)<sup>29</sup>. All knees with KLG < 2 were excluded from the analyses.

## *2.3. Optical motion capture*

Ground reaction force (GRF) and kinematic data were collected from both legs for all participants while walking along a 15-meter walkway at self-selected and fast speeds. A passive optical motion capture system with 12 infrared cameras and one video camera (Qualisys Medical, Gothenburg, Sweden) was used to capture kinematic data at 250 Hz. Twenty-six spherical retroreflective markers were attached to bony landmarks of the trunk (manubrium, C7 spinous process, T8 spinous process, and the right and left acromion), pelvis (right and left anterior superior iliac spines, superior aspects of iliac crests, right and left posterior superior iliac spines, and sacrum), and lower extremities (greater trochanters, lateral and

medial femoral epicondyles, lateral and medial malleoli, first and fifth metatarsal heads) which were used to identify joint centers during a static standing trial (Figure 1A). Rigid clusters of four markers were placed on the shank and thigh segments, and markers were placed on the posterior aspect of the heel, medial and lateral mid-foot, 2<sup>nd</sup> metatarsal head, and lateral aspect of 5<sup>th</sup> metatarsal head for segment tracking (Figure 1A). Three force platforms (AMTI, Watertown, MA, USA) were used to collect GRF data at 2000 Hz synchronously with the motion data. Walking speed was measured using a timing system (Brower Timing Systems, Draper, UT, USA). Self-selected and fast walking target speeds were determined after 3-4 practice trials. For self-selected speed trials, participants were instructed to “walk across the room towards the door with a purposeful pace.” For fast walking trials, participants were instructed to “walk as quickly as you comfortably can without running and without going faster than what you feel is safe for you.” Any trials that were outside  $\pm 5\%$  of the target walking speeds were excluded. Four to six clean force plate foot strikes were collected for each foot. Each participant wore laboratory-provided shoes (Gel-Cumulus 19, ASICS, Kobe, Japan).

Within the motion capture software, marker trajectories were identified and any gaps in data were filled using polynomial splines for gaps of less than 10 frames and trajectory matching for larger gaps. All data were then imported into Visual3D (C-Motion, Germantown, MD, USA). Marker and GRF data were filtered using low-pass, 4th order Butterworth filters with cut-off frequencies of 6 Hz and 12 Hz, respectively, as the majority of movement during walking occurs below these frequencies. Joint kinematics were calculated from the marker data using Euler angles (x-y-z) and right-handed coordinate systems. Initial and final contact for each clean foot strike were identified from the GRF using a threshold of 20 N to define stance phase.

The primary measure from the optical motion capture system was peak knee adduction velocity and the secondary measure was knee adduction excursion. Chang et al. suggested peak knee adduction velocity as an appropriate biomechanical index to quantify varus thrust as it closely corresponded with

visual assessments and captures both the direction and speed of movement<sup>6</sup>. As the majority of the varus thrust movement occurs in early stance<sup>6</sup>, peak knee adduction velocity during the first half of stance phase was recorded (Figure 2B). It should be noted that because the joint angle (Euler angle) is a vector quantity, it is not possible to compute the joint angular velocity by taking the first derivative of the joint angle<sup>30</sup>. We used X-Y-Z cardan sequence to calculate the knee joint angle (shank relative to thigh); the knee joint angular velocity was calculated as the angular velocity of the shank relative to the thigh<sup>30,31</sup>. The secondary motion capture varus thrust measure, knee adduction excursion, was calculated as the difference between the knee adduction angle at initial contact and the maximum knee adduction angle during the first half of stance<sup>6</sup> (Figure 2C). Inverse dynamics were used to calculate the EKAM, normalized to body weight and height (% bodyweight-height), and the peak EKAM was extracted from the first half of stance (Figure 2D). All variables were averaged across all clean foot strikes for each leg.

#### *2.4. Inertial motion capture*

Small, lightweight inertial sensors (Trigno<sup>TM</sup> IM Sensor, Delsys, Inc., Natick, MA, USA) were used concurrently with the optical motion capture system. Each sensor measured 37mm x 26mm x 15mm, weighed 14.7g, and consisted of a triaxial accelerometer ( $\pm 16g$ ), a triaxial gyroscope ( $\pm 2000$  degree/s), and a triaxial magnetometer ( $\pm 1000\mu T$ ). Initially, three sensor locations were tested for each limb (Figure 1B): 1) lateral mid-thigh (attached to the thigh segment optical motion capture marker cluster), 2) lateral mid-shank (attached to the shank segment optical motion capture marker cluster), and 3) lateral distal shank (attached directly to the skin on the lateral aspect of the distal tibia proximal to the lateral malleolus). The distal shank placement was included with the assumption that it would be more convenient for use in a non-laboratory environment. However, interim analyses showed poor association between optical motion capture data and data from the distal sensor, particularly during fast

speed walking, and this sensor was perceived as uncomfortable by a few participants. For these reasons, use of the distal sensor placement was discontinued for the final 11 participants (22 knees) enrolled in this study and the data from this sensor are not presented here. For all sensor placements, while a general orientation of the sensors was specified (i.e. arrow side 'up'), the placement along the length of the leg and anterior-posterior position were not constrained, nor were any calibration procedures performed, in order to better replicate placement of the sensors in a clinical setting and/or by untrained individuals (e.g. participants).

Data were recorded from each sensor at 148 Hz, upsampled to 2000 Hz, and time synchronized with the optical motion capture system. The frontal plane component of the raw gyroscope data was used as a measure of segment adduction velocity. The gyroscope component was chosen as it captures angular velocity as compared to accelerometer components which capture linear acceleration. Peak segment adduction velocity in degrees per second, which was calculated as the peak value between initial contact and midstance, was extracted for each trial for each sensor (Figure 2A) and averaged across trials for each leg. Outcomes used in the analyses included peak thigh adduction velocity from the mid-thigh sensor (mid-thigh adduction velocity) and peak shank adduction velocity from the mid-shank sensor (mid-shank adduction velocity) for each walking speed. It should be noted that the thigh adduction velocity is recorded as positive and shank adduction velocity is recorded as negative (Figure 2, Table 2) given the nature of segmental motion and orientation of the sensor coordinate systems (Figure 1B).

## *2.5. Statistical Analyses*

For the primary aim, univariate regression models with generalized estimating equations (GEE) were used to assess the relationships between the inertial sensor measures and the optical motion capture measures, separately for self-selected and fast speed walking. The GEEs allowed us to account the

correlation between knees within each person. For the secondary aim, multivariate regression models with GEE were used to assess the relationships between EKAM and the inertial sensor measures, separately for each speed, while adjusting for a number of confounders (specifically age, sex, BMI, KLG, and static alignment) that may affect both varus thrust<sup>13</sup> and EKAM<sup>32–34</sup>. While pain can also affect EKAM<sup>32</sup>, we hypothesized that it acts as a mediator rather than a confounder on the causal pathway (i.e. varus thrust causes pain rather than the other way around), and thus did not include it in the models. All models were constructed including a term for leg and an interaction term between exposure and leg to determine whether the association of the exposure and the outcome differed by leg. If there was no interaction between exposure and leg (i.e. this interaction term was not significant), the model was re-run without the exposure by leg interaction term. All analyses were performed using IBM SPSS (Armonk, NY, USA) in all knees with KLG  $\geq 2$ . Significance was set at  $\alpha = 0.05$ .

### 3. Results

One hundred and sixty-three individuals underwent telephone screening, 82 passed the initial screening process, 59 underwent a radiographic screening visit, and 26 individuals (16 female) were deemed eligible for this study (Figure 3, Table 1). The number of knees across analyses differed depending on useable data available for each inertial sensor (Figure 3). Average values for each inertial and optical motion capture measure are reported in Table 2.

Both mid-thigh and mid-shank adduction velocity were associated with knee adduction velocity and excursion during self-selected and fast speed walking. An increase of  $10.0^\circ/\text{s}$  in mid-thigh adduction velocity was associated with an increase in knee adduction velocity of  $6.1^\circ/\text{s}$  during self-selected speed walking ( $P < 0.001$ , Figure 4A) and  $5.3^\circ/\text{s}$  during fast walking ( $P = 0.001$ , Figure 4B), and an increase in knee adduction excursion of  $0.35^\circ$  during self-selected speed walking ( $P = 0.005$ , Figure 4C) and  $0.33^\circ$  during fast walking ( $P = 0.020$ , Figure 4D). Similarly, an increase of  $10.0^\circ/\text{s}$  in mid-shank adduction

velocity was associated with an increase in knee adduction velocity of  $3.4^{\circ}/s$  during self-selected speed walking ( $P < 0.001$ , Figure 4A) and  $2.2^{\circ}/s$  during fast walking ( $P = 0.005$ , Figure 4B), and an increase in knee adduction excursion of  $0.20^{\circ}$  during both self-selected ( $P = 0.004$ , Figure 4C) and fast ( $P < 0.001$ , Figure 4D) speed walking.

After accounting for age, sex, BMI, KLG, and static alignment, an increase of  $10.0^{\circ}/s$  in mid-thigh adduction velocity was associated with an increase in EKAM of 0.16 % bodyweight-height ( $P < 0.001$ ) during self-selected speed walking and an increase of 0.17 % bodyweight-height ( $P < 0.001$ ) during fast speed walking. For the models investigating the relationship between mid-shank adduction velocity and EKAM during self-selected and fast speed walking, the interaction term between leg and mid-shank adduction velocity was significant, thus separate models were run for left and right legs. For left legs ( $n = 18$ ), an increase in  $10.0^{\circ}/s$  in mid-shank adduction velocity was associated with an increase in EKAM of 0.10 % bodyweight-height ( $P = 0.010$ ) during self-selected speed walking and an increase in 0.17 % bodyweight-height ( $P < 0.001$ ) during fast speed walking, after accounting for confounders. For right legs ( $n = 23$ ), mid-shank adduction velocity was not associated with EKAM at either self-selected speed ( $P = 0.88$ ) or fast speed ( $P = 0.21$ ).

#### 4. Discussion

This proof-of-concept study showed that the measures from single inertial sensors were associated with surrogate measures of varus thrust obtained using optical motion capture. Furthermore, supporting our secondary hypothesis, mid-thigh adduction velocity was significantly associated with peak EKAM after adjusting for confounders. These results suggest that inertial sensors should be further investigated as a tool to objectively quantify varus thrust in clinical settings where optical motion capture is not feasible and visual assessment is insufficient. The ability to quickly and accurately quantify varus thrust in clinical

or other real-world settings could lead to better identification and treatment of those at risk of OA progression due to varus thrust.

Both inertial sensor metrics – mid-thigh adduction velocity and mid-shank adduction velocity – were associated with both optical motion capture thrust measures at both walking speeds. The mid-shank data, however, had greater variability than the mid-thigh data, e.g. an adduction velocity range of 165°/s for the mid-shank versus 99°/s for the mid-thigh during self-selected speed walking (Figure 4, Table 2), suggesting that the mid-thigh sensor placement is superior. These results are supported by previous research that found data from a single mid-thigh inertial sensor were a better predictor of peak knee extensor moment and power absorption during a single limb task than a mid-shank sensor<sup>35</sup> and that data from a single thigh accelerometer, but not a single shank accelerometer, were predictive of between-limb differences in knee power absorption during running<sup>36</sup>.

In the current study, both of the mid-segment inertial sensors were placed directly on the rigid optical motion capture marker clusters used for segment tracking. However, it is the anatomical coordinate system defined by markers placed on bony landmarks, rather than these rigid clusters, that define the segment coordinate systems for the motion capture measures. Orientation of the inertial sensors relative to the anatomical coordinate system is a key factor in accuracy of joint angles measured by inertial sensors<sup>37</sup>. A varying degree of curvature on the lateral aspect of the shank due to the shape of the lateral head of the gastrocnemius muscle could have resulted in less consistent placement of the mid-shank inertial sensor among legs, thus affecting the relationship between the inertial sensor coordinate system and the anatomical coordinate system of the shank. In contrast, the lateral thigh has less variation in curvature along its length, which may have ensured more consistent placement of the mid-thigh inertial sensor across legs. Thus, the mid-thigh sensor placement may be preferable to the mid-shank placement for assessing varus thrust in individuals with knee OA, particularly in cases where limited time or experience prevent more standardized placement.

The regression models for EKAM also provide support for the mid-thigh versus mid-shank placement as the association between segment angular velocity and EKAM was not consistent across legs for the mid-shank sensor, i.e. it was significant for the left but not the right leg. While the current dataset did not provide enough power for a thorough comparison between left and right legs, these groups were similar in terms of KLG and HKA, thus no difference between legs was expected. Despite this discrepancy between legs for the mid-shank sensor, the novel finding that mid-thigh adduction velocity was significantly associated with EKAM, even after adjusting for confounders, is promising as it suggests that an estimation of EKAM may be possible without the need for extensive laboratory equipment or analysis of multiple inertial sensors. This finding also supports previous studies that have shown associations between various quantitative measures of varus thrust and EKAM<sup>17,20,21</sup>.

In the current study, only single-sensor inertial measures were examined with the idea that large-scale screening in a clinical setting would require a quick set-up with minimal data processing. However, the lack of an exact 1:1 increase in adduction velocity between these inertial sensor and optical motion captures measures may be attributed to the fact that the inertial sensor segment adduction velocity measures only describe movement of a single segment (thigh or shank), while knee adduction velocity describes the relative movement between the thigh and shank segments. Integration of multiple inertial sensors or sensor components may result in better estimation of knee adduction velocity, however, this typically requires a series of functional calibration exercises, modeling assumptions, and data filtering to address issues such as drift and sensor alignment<sup>38</sup>. The finding in the current study of a significant association between single inertial sensor measures and optical motion capture measures suggests a single sensor may be sufficient as a quick screening tool for severity of varus thrust in knee OA populations where more extensive data collection is not feasible.

We observed significant associations of mid-thigh and mid-shank sensors with both knee adduction velocity and knee adduction excursion measures at both walking speeds. As noted by Chang

et al.<sup>6</sup>, knee adduction velocity captures the speed of the movement and can be used as a reliable measure of varus thrust in people with knee OA. Knee adduction excursion has also been used as a quantitative metric of varus thrust and has been associated with both OA severity (KLG) and EKAM in individuals with medial knee OA<sup>21</sup>. Associations would be expected between measures of thigh/shank adduction velocity from the inertial sensors and knee adduction velocity from optical motion capture given the similar constructs being measured. However, significant associations of metrics from thigh/shank inertial sensors and knee adduction excursion further support the use of inertial sensors to assess varus thrust. Furthermore, the similarity of results across the two speeds for the analyses in the current study suggests that a single sensor could be used to quantify varus thrust across different walking speeds in individuals with knee OA.

There are a number of limitations of the current study that should be acknowledged. Given that this was a proof of concept study, the sample size was small. Data error resulted in the loss of inertial sensor data for some legs due to signal clipping. While this appeared to be an issue with software presets, rather than the inertial sensors themselves, the loss of this data and small sample size overall did not provide enough power for a definitive comparison across sensor locations or speeds. The lack of standardized placement of the inertial sensors on the leg, e.g. a specified percent distance along a given segment, may have increased variability in the measurement of segment adduction velocities from the inertial sensors, resulting in misalignment of coordinate systems between the inertial and optical motion capture systems and an inability to provide a definitive recommendation on sensor placement. The attachment of sensors in a clinical setting would likely also be done without standardized placement or calibration and thus these results may be a good representation of how clinical inertial sensor data would correspond to optical motion capture data. It should be noted, however, that the sensors in the current study were placed on top of the rigid plate containing optical motion capture markers and it is unclear whether a rigid sensor alone versus the rigid sensor/plate combination would produce similar

data. In this study, gait events identified by the optical motion capture system were used for calculation of the inertial measures. In a clinical setting where optical motion capture data are not available, gait events calculated from the inertial sensors, as has been done previously<sup>39</sup>, would need to be utilized. Reliability of the thigh inertial sensor measurement will also need to be established before it can be used in clinical settings, particularly given the limited number of studies investigating reliability of inertial sensors in knee OA populations<sup>40,41</sup>. It should also be noted that while the sample in the current study is similar to that of larger studies of individuals with medial knee OA in terms of age, sex, and BMI<sup>13</sup>, the results may not generalize to other sub-groups of the OA population such as individuals with BMI > 40.

## **5. Conclusions**

In this proof-of-concept study, we demonstrated a significant association between increases in thigh angular velocity derived from the gyroscope signal of a single inertial sensor and increases in surrogate varus thrust measures derived from an optical motion capture system. Furthermore, increased thigh angular velocity from this single inertial sensor was associated with increased peak EKAM after adjusting for confounders. These results highlight the potential of inertial sensors for quantifying varus thrust without the need for an optical motion capture system.

## **Acknowledgments**

We would like to acknowledge the staff and students of the Movement & Applied Imaging Laboratory for their contributions to data collection and processing. We would also like to thank the participants for their contributions to this study and ASICS for donating the shoes used in this study.

330           Research reported in this publication was supported by the National Institutes of Health, under  
331   award numbers K01AR069720 and T32AR007598. The content is solely the responsibility of the authors  
332   and does not necessarily represent the official views of the National Institutes of Health.

333

## References

1. Guccione A, Felson DT, Anderson JJ, et al. The effects of specific medical conditions on the functional limitations of elders in the Framingham study. *Am J Public Health*. 1994;84(3):351-358.
2. McAlindon TE, Snow S, Cooper C, Dieppe PA. Radiographic patterns of osteoarthritis of the knee joint in the community: The importance of the patellofemoral joint. *Ann Rheum Dis*. 1992;51:844-849. doi:10.1136/ard.51.7.844
3. Felson DT, Lawrence RC, Dieppe PA, et al. Osteoarthritis: New insights - Part 1: The disease and its risk factors. *Ann Intern Med*. 2000. doi:10.7326/0003-4819-133-8-200010170-00016
4. Wink AE, Gross KD, Brown CA, et al. Varus thrust during walking and the risk of incident and worsening medial tibiofemoral MRI lesions: the Multicenter Osteoarthritis Study. *Osteoarthritis Cartil*. 2017;25(6):839-845.
5. Chang A, Hayes K, Dunlop D, et al. Thrust during ambulation and the progression of knee osteoarthritis. *Arthritis Rheum*. 2004;50(12):3897-3903. doi:10.1002/art.20657
6. Chang AH, Chmiel JS, Moision KC, et al. Varus thrust and knee frontal plane dynamic motion in persons with knee osteoarthritis. *Osteoarthritis Cartil*. 2013;21(11):1668-1673.
7. Lo GH, Harvey WF, McAlindon TE. Associations of varus thrust and alignment with pain in knee osteoarthritis. *Arthritis Rheum*. 2012;64(7):2252-2259. doi:10.1002/art.34422
8. Hurwitz DE, Sumner DR, Andriacchi TP, Sugar DA. Dynamic knee loads during gait predict proximal tibial bone distribution. *J Biomech*. 1998;31(5):423-430. doi:10.1016/S0021-9290(98)00028-1
9. Chang AH, Moision KC, Chmiel JS, et al. External knee adduction and flexion moments during gait and medial tibiofemoral disease progression in knee osteoarthritis. *Osteoarthritis Cartil*.

- 2015;23(7):1099-1106. doi:10.1016/j.joca.2015.02.005
10. Iijima H, Fukutani N, Aoyama T, et al. Clinical phenotype classifications based on static varus alignment and varus thrust in Japanese patients with medial knee osteoarthritis. *Arthritis Rheumatol.* 2015;67(9):2354-2362.
11. Iijima H, Fukutani N, Yamamoto Y, et al. Association of varus thrust with prevalent patellofemoral osteoarthritis: A cross-sectional study. *Gait Posture.* 2017;58:394-400. doi:10.1016/j.gaitpost.2017.08.033
12. Fukutani N, Iijima H, Fukumoto T, et al. Association of varus thrust with pain and stiffness and activities of daily living in patients with medial knee osteoarthritis. *Phys Ther.* 2016;96(2):167-175. doi:10.2522/ptj.20140441
13. Chang A, Hochberg M, Song J, et al. Frequency of varus and valgus thrust and factors associated with thrust presence in persons with or at higher risk of developing knee osteoarthritis. *Arthritis Rheum.* 2010;62(5):1403-1411. doi:10.1002/art.27377
14. Sharma L, Chang AH, Jackson RD, et al. Varus thrust and incident and progressive knee osteoarthritis. *Arthritis Rheumatol.* 2017. doi:10.1002/art.40224
15. Fukaya T, Mutsuzaki H, Wadano Y. Kinematic analysis of knee varus and rotation movements at the initial stance phase with severe osteoarthritis of the knee. *Knee.* 2015;22(3):213-216. doi:10.1016/j.knee.2015.02.012
16. Kakihana W, Akai M, Nakazawa K, Naito K, Torii S. Inconsistent knee varus moment reduction caused by a lateral wedge in knee osteoarthritis. *Am J Phys Med Rehabil.* 2007;86(6):446-454. doi:10.1097/PHM.0b013e31805bfff5
17. Mahmoudian A, van Dieen JH, Bruijn SM, et al. Varus thrust in women with early medial knee

378 osteoarthritis and its relation with the external knee adduction moment. *Clin Biomech.*  
379 2016;39:109-114. doi:10.1016/j.clinbiomech.2016.10.006

380 18. Brown TN, Kaplan JT, Cameron SE, Seymore KD, Ramsay JW. Individuals with varus thrust do not  
381 increase knee adduction when running with body borne load. *Journal of Biomechanics.* 2018.

382 19. Hunt MA, Schache AG, Hinman RS, Crossley KM. Varus thrust in medial knee osteoarthritis:  
383 Quantification and effects of different gait-related interventions using a single case study.  
384 *Arthritis Care Res.* 2011;63(2):293-297. doi:10.1002/acr.20341

385 20. Sosdian L, Hinman RS, Wrigley T V., et al. Quantifying varus and valgus thrust in individuals with  
386 severe knee osteoarthritis. *Clin Biomech.* 2016;39:44-51. doi:10.1016/j.clinbiomech.2016.09.007

387 21. Kuroyanagi Y, Nagura T, Kiriya Y, et al. A quantitative assessment of varus thrust in patients  
388 with medial knee osteoarthritis. *Knee.* 2012;19(2):130-134. doi:10.1016/j.knee.2010.12.007

389 22. Brodie MAD, Coppens MJM, Lord SR, et al. Wearable pendant device monitoring using new  
390 wavelet-based methods shows daily life and laboratory gaits are different. *Med Biol Eng Comput.*  
391 2016;54(4):663-674. doi:10.1007/s11517-015-1357-9

392 23. Tao W, Liu T, Zheng R, Feng H. Gait analysis using wearable sensors. *Sensors.* 2012;12(2):2255-  
393 2283. doi:10.3390/s120202255

394 24. Konrath JM, Karatsidis A, Schepers HM, Bellusci G, de Zee M, Andersen MS. Estimation of the  
395 Knee Adduction Moment and Joint Contact Force during Daily Living Activities Using Inertial  
396 Motion Capture. *Sensors.* 2019;19. doi:10.3390/s19071681

397 25. Zügner R, Tranberg R, Timperley J, Hodgins D, Mohaddes M, Kärrholm J. Validation of inertial  
398 measurement units with optical tracking system in patients operated with Total hip arthroplasty.  
399 *BMC Musculoskelet Disord.* 2019;20(1). doi:10.1186/s12891-019-2416-4

- 400 26. Altman R, Asch E, Bloch D, et al. Development of criteria for the classification and reporting of  
401 osteoarthritis: Classification of osteoarthritis of the knee. *Arthritis Rheumatol.* 1986;29(8):1039-  
402 1049. doi:10.1002/art.1780290816
- 403 27. Guermazi A, Hayashi D, Roemer F, et al. Severe radiographic knee osteoarthritis - does Kellgren  
404 and Lawrence grade 4 represent end stage disease? - the MOST study. *Osteoarthr Cartil.*  
405 2015;23(9):1499-1505. doi:10.1016/j.joca.2015.04.018
- 406 28. Rosset A, Spadola L, Ratib O. OsiriX: An open-source software for navigating in multidimensional  
407 DICOM images. *J Digit Imaging.* 2004;17(3):205-216. doi:10.1007/s10278-004-1014-6
- 408 29. Roos EM, Roos HP, Lohmander LS, Ekdahl C, Beynnon BD. Knee Injury and Osteoarthritis  
409 Outcome Score (KOOS)—Development of a self-administered outcome measure. *J Orthop Sport*  
410 *Phys Ther.* 1998;28(2):88-96. doi:10.2519/jospt.1998.28.2.88
- 411 30. Hamill J, Selbie W, Kepple T. Three-dimensional kinematics. In: Robertson DGE, Caldwell GE,  
412 Hamill J, Kamen G, Whittlesey SN, eds. *Research Methods in Biomechanics*. 2nd ed. Champaign,  
413 IL, USA; 2013:35-60.
- 414 31. C-Motion. Joint Velocity. [https://c-motion.com/v3dwiki/index.php/Joint\\_Velocity](https://c-motion.com/v3dwiki/index.php/Joint_Velocity). Accessed  
415 October 13, 2020.
- 416 32. Hurwitz DE, Ryals AB, Case JP, Block JA, Andriacchi TP. The knee adduction moment during gait in  
417 subjects with knee osteoarthritis is more closely correlated with static alignment than  
418 radiographic disease severity, toe out angle and pain. *J Orthop Res.* 2002;20(1):101-107.  
419 doi:10.1016/S0736-0266(01)00081-X
- 420 33. Blazek K, Asay JL, Erhart-Hledik J, Andriacchi T. Adduction moment increases with age in healthy  
421 obese individuals. *J Orthop Res.* 2013;31(9):1414-1422. doi:10.1002/jor.22390

34. Sims EL, Carland JM, Keefe FJ, Kraus VB, Guilak F, Schmitt D. Sex differences in biomechanics associated with knee osteoarthritis. *J Women Aging*. 2009;21(3):159-170. doi:10.1080/08952840903054856
35. Pratt KA, Sigward SM. Inertial sensor angular velocities reflect dynamic knee loading during single limb loading in individuals following anterior cruciate ligament reconstruction. *Sensors (Switzerland)*. 2018;18(10). doi:10.3390/s18103460
36. Havens KL, Cohen SC, Pratt KA, Sigward SM. Accelerations from wearable accelerometers reflect knee loading during running after anterior cruciate ligament reconstruction. *Clin Biomech*. 2018;58(July):57-61. doi:10.1016/j.clinbiomech.2018.07.007
37. Kianifar R, Joukov V, Lee A, Raina S, Kulić D. Inertial measurement unit-based pose estimation: Analyzing and reducing sensitivity to sensor placement and body measures. *J Rehabil Assist Technol Eng*. 2019;6:205566831881345. doi:10.1177/2055668318813455
38. Seel T, Raisch J, Schauer T. IMU-based joint angle measurement for gait analysis. *Sensors*. 2014;14(4):6891-6909. doi:10.3390/s140406891
39. Aminian K, Najafi B, Büla C, Leyvraz P-F, Robert P. Spatio-temporal parameters of gait measured by an ambulatory system using miniature gyroscopes. *J Biomech*. 2002;35(5):689-699. doi:10.1016/S0021-9290(02)00008-8
40. Kobsar D, Osis ST, Phinyomark A, Boyd JE, Ferber R. Reliability of gait analysis using wearable sensors in patients with knee osteoarthritis. *J Biomech*. 2016;49(16):3977-3982. doi:10.1016/j.jbiomech.2016.11.047
41. Turcot K, Aissaoui R, Boivin K, Hagemeister N, Pelletier M, Guis JA d. Test-retest reliability and minimal clinical change determination for 3-dimensional tibial and femoral accelerations during treadmill walking in knee osteoarthritis patients. *Arch Phys Med Rehabil*. 2008;89(4):732-737.

445           doi:10.1016/j.apmr.2007.09.033

446

447

448 Table 1. Sample characteristics

Clinical & Demographic Characteristics	n = 26 participants†
Sex	n = 16 [62%] female
Age (years)	64.5 (8.4)
Body mass index (kg/m <sup>2</sup> )	28.6 (4.7)
Height (m)	1.67 (0.12)
Gait speed (m/s):	
Self-selected	1.32 (0.22)
Fast	1.62 (0.32)
Knee Injury and Osteoarthritis Outcome Score - Pain (/100*)	59.2 (11.1)
Kellgren-Lawrence Grade (KLG):	
KLG = 2	n = 13 legs
KLG = 3	n = 26 legs
KLG = 4	n = 8 legs
Static limb alignment (degrees)**	175.9 (3.6)

*Data presented as mean (standard deviation) except where noted*

*†n = 47 knees from these participants had KLG ≥ 2. KOOS, KLG, & alignment values are reported for these knees only.*

*\*Lower scores represent greater pain*

*\*\*Angles < 180 degrees indicate static varus alignment*


449

450

451 Table 2: Inertial and optical motion capture outcome average values in knees with radiographic OA (KLG  
 452  $\geq 2$ )

<b>Inertial motion capture</b>	
Mid-thigh adduction velocity (degree/s) (n = 39 legs):	
Self-selected speed walking	45.2 (25.2)
Fast speed walking	58.9 (28.1)
Mid-shank adduction velocity (degree/s) (n = 41 legs):	
Self-selected speed walking	-80.4 (36.9)
Fast speed walking	-97.3 (43.4)
<b>Optical motion capture</b>	
Knee adduction velocity (degree/s) (n = 45 legs):	
Self-selected speed walking	63.9 (24.8)
Fast speed walking	75.6 (28.6)
Knee adduction excursion (degree) (n = 45 legs):	
Self-selected speed walking	3.8 (2.0)
Fast speed walking	4.0 (2.1)
External knee adduction moment (% bodyweight-height) (n = 45 legs):	
Self-selected speed walking	3.25 (1.22)
Fast speed walking	3.71 (1.43)
<i>Data presented as mean (standard deviation)</i>	

453

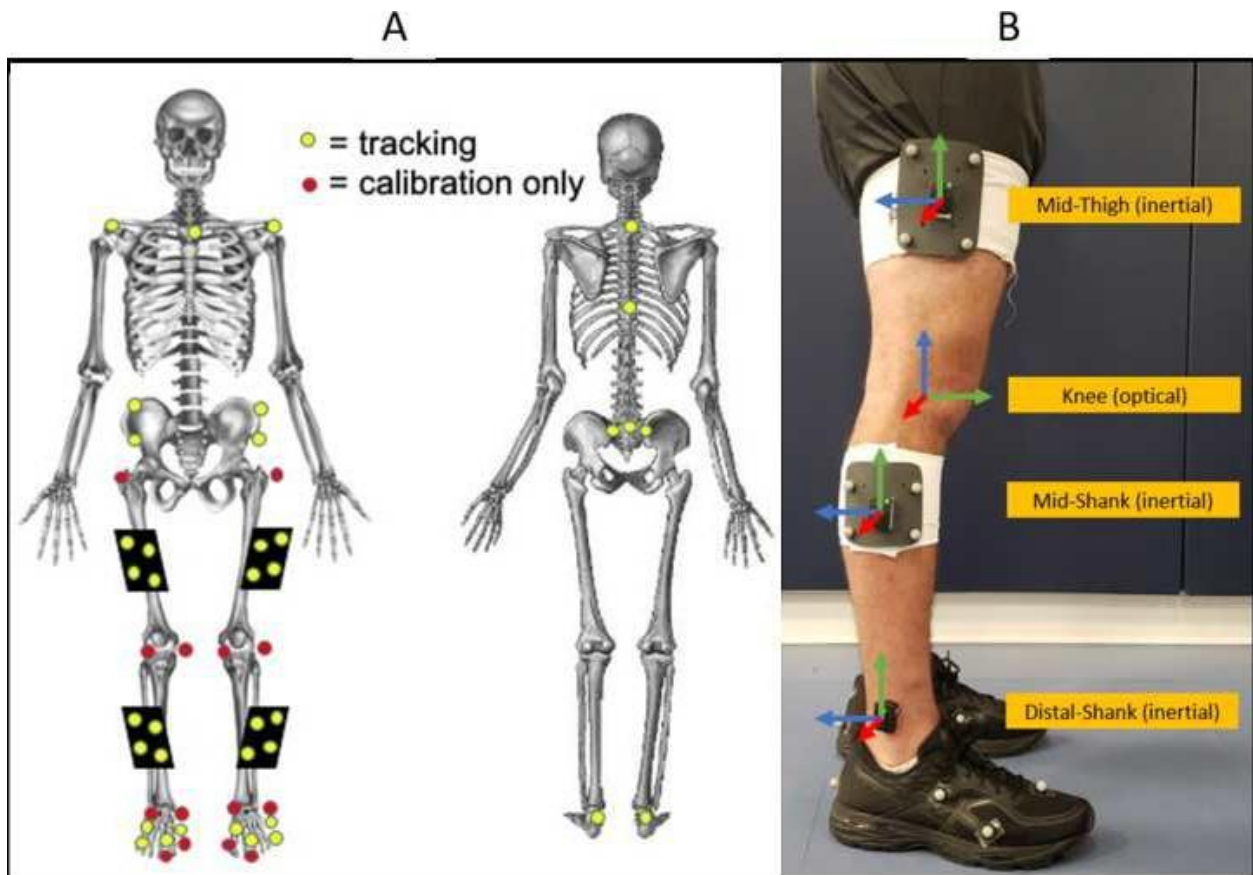

454

455

456

457

458

459

Figure 1. (A) Optical motion capture markers (red markers used for static trial only) and (B) inertial sensors, showing placement of the mid-thigh and mid-shank inertial sensors on the optical motion capture marker clusters for the thigh and shank segments, respectively, and distal shank inertial sensor directly on the skin on the lateral aspect of the distal tibia, along with the coordinate systems for the knee (optical system) and inertial sensors.

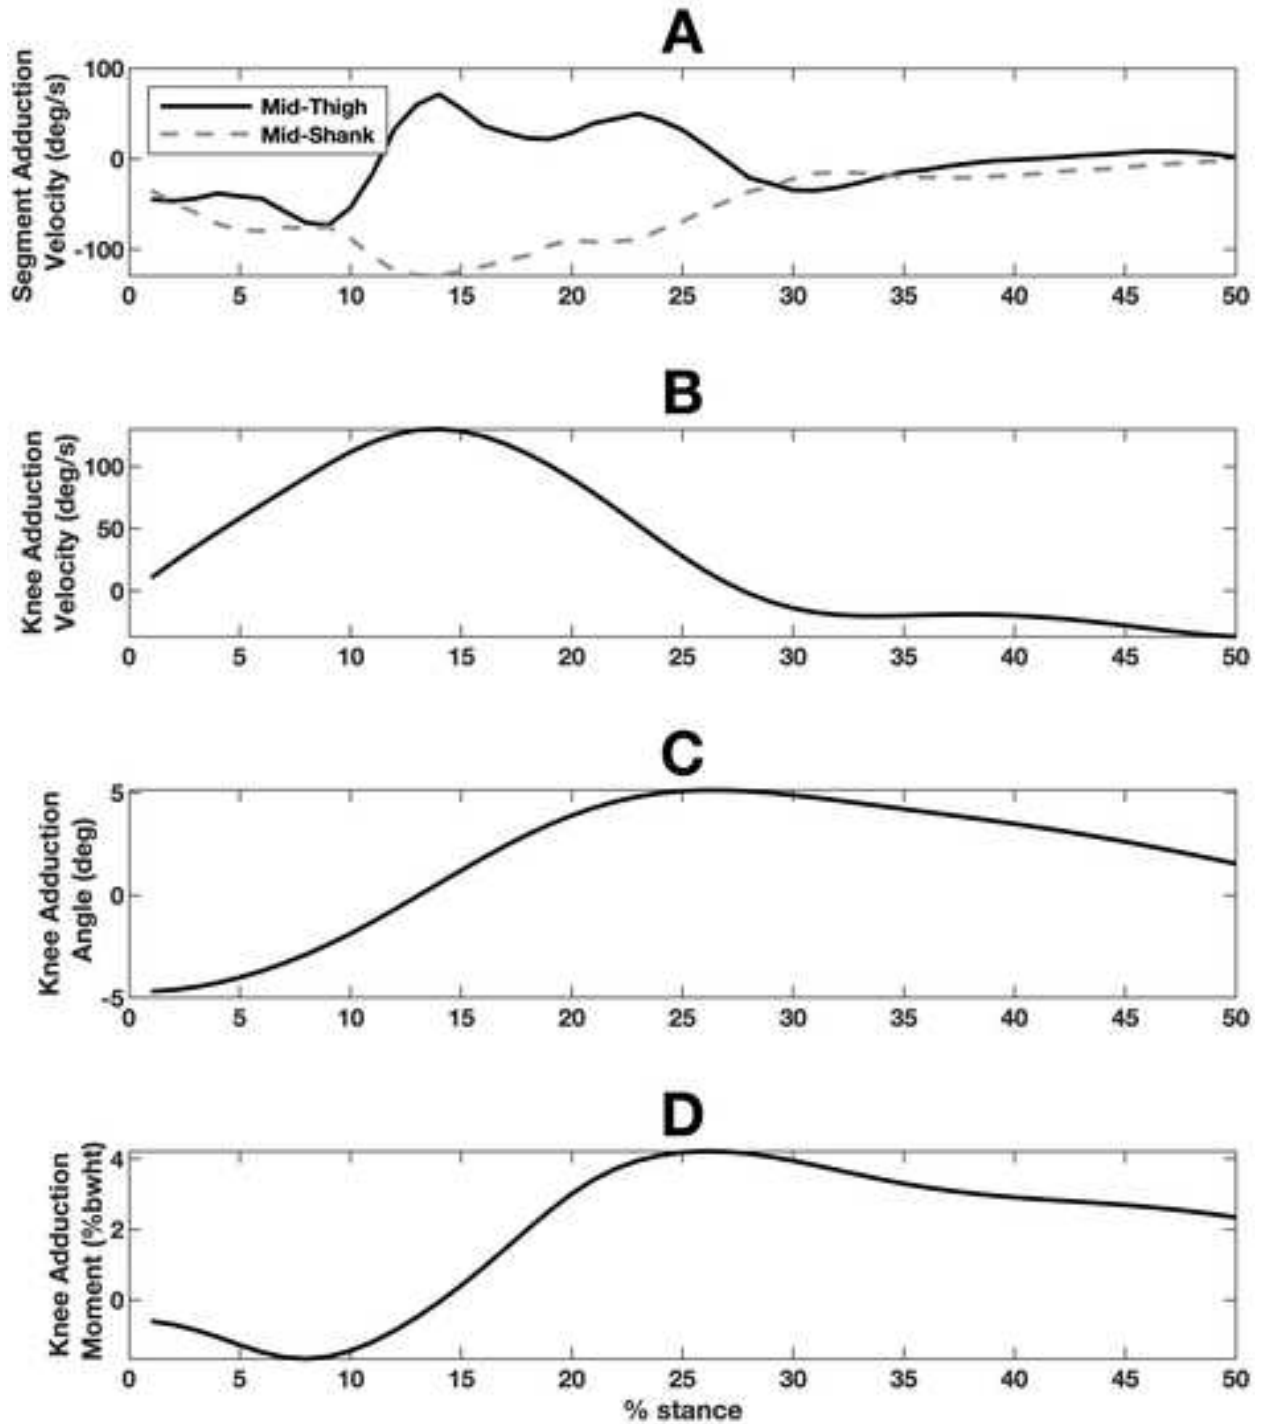


Figure 2. Representative waveforms from self-selected speed walking showing (A) inertial sensor segment adduction velocity from the mid-thigh and mid-shank sensors, (B) knee adduction velocity, (C) knee adduction angle and knee adduction excursion, and (D) external knee adduction moment (EKAM).

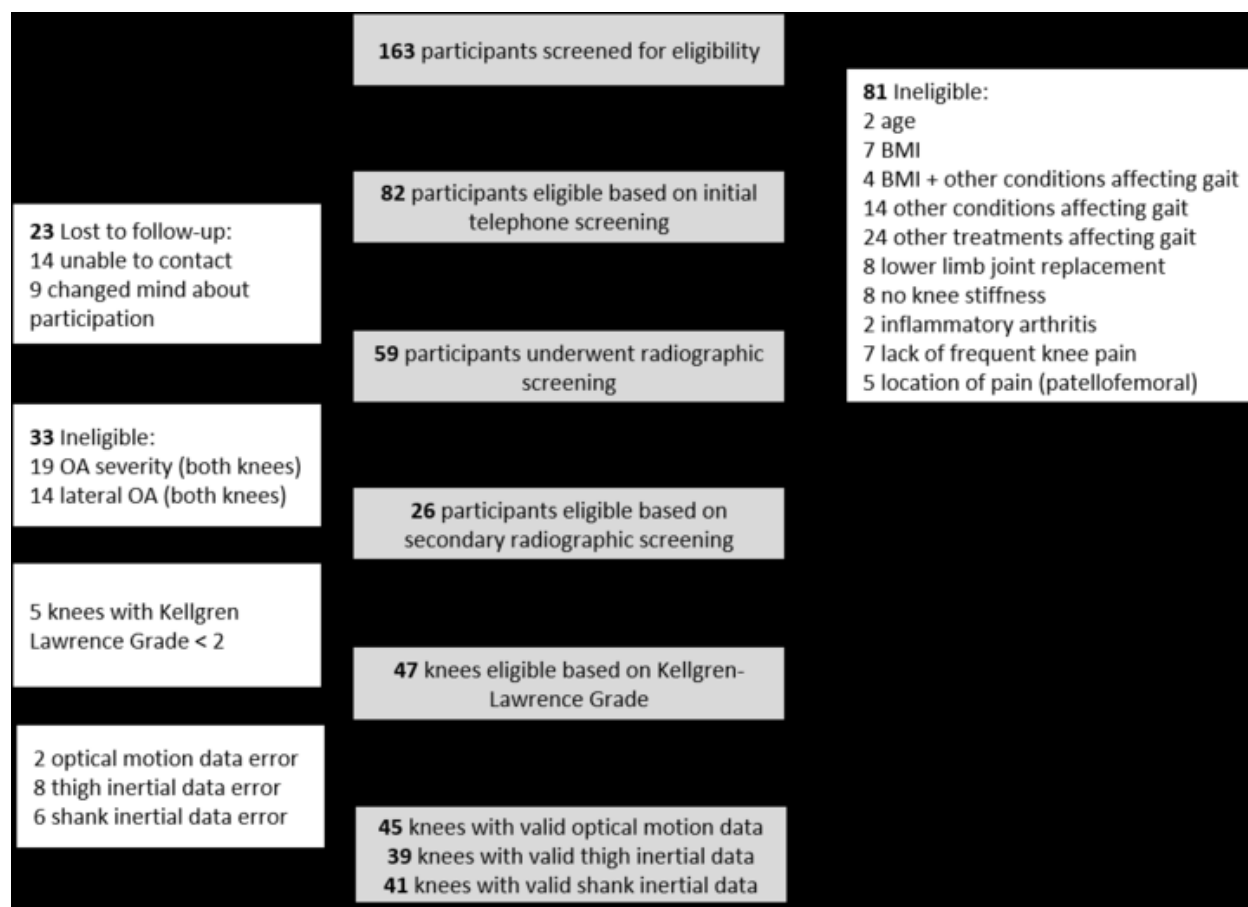


Figure 3. Study recruitment and final study sample.

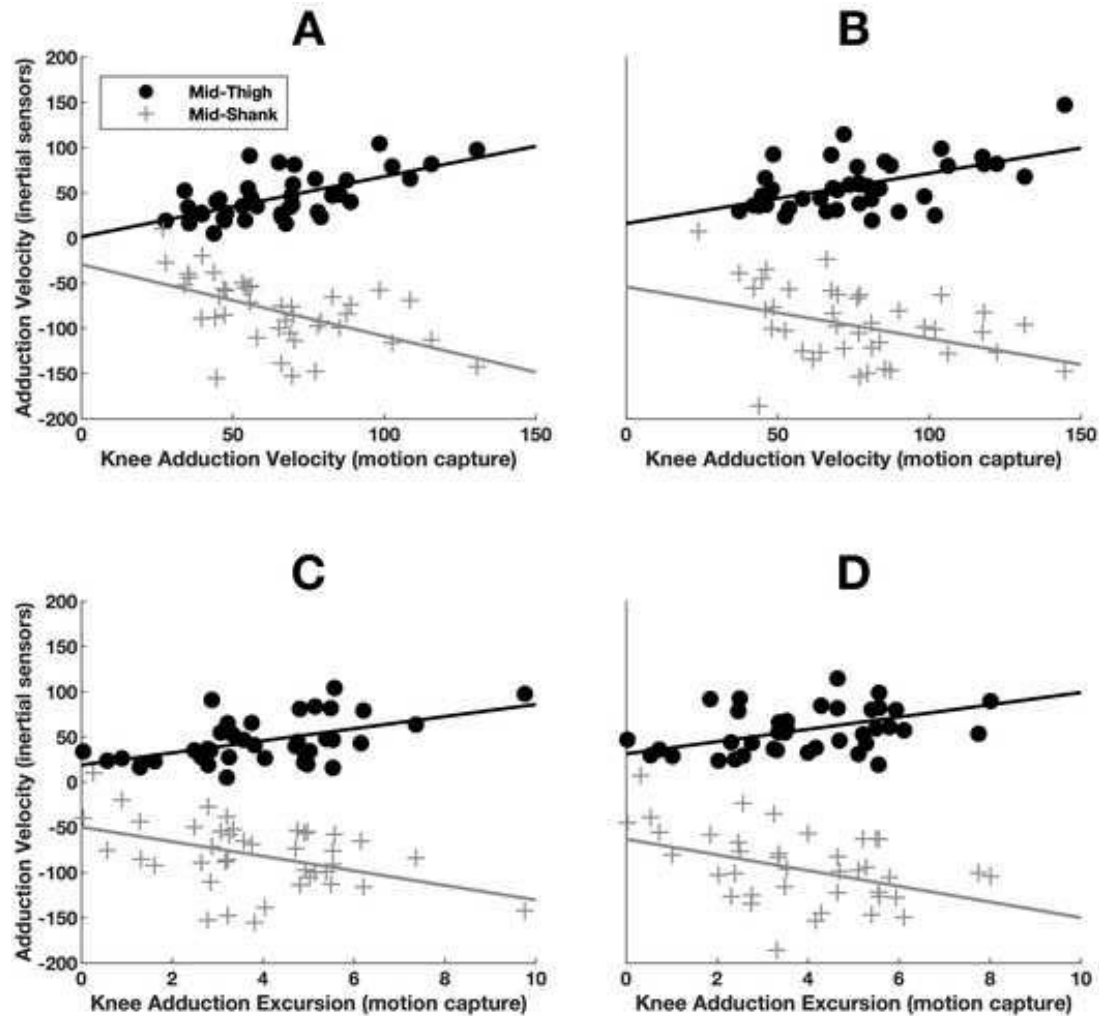


Figure 4. Relationships between segment adduction velocity (captured by the inertial sensors) and (A) knee adduction velocity during self-selected speed walking, (B) knee adduction velocity during fast speed walking, (C) knee adduction excursion during self-selected speed walking, and (D) knee adduction excursion during fast speed walking in knees with radiographic osteoarthritis.